



POSTERIOR CROWNS

PROCERA® ALUMINA/ZIRCONIA, CERCON® ZIRCONIA, LAVA® ZIRCONIA

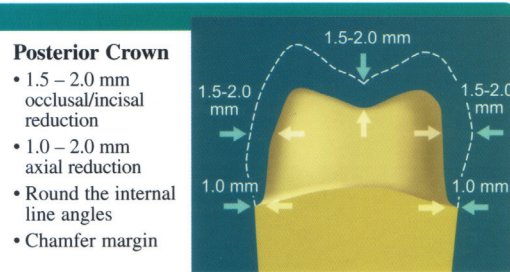


POSTERIOR BRIDGES

PROCERA® ALUMINA/ZIRCONIA, CERCON® ZIRCONIA, LAVA® ZIRCONIA

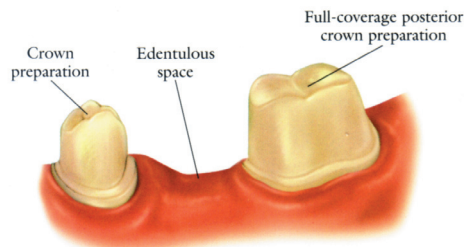

ANTERIOR CROWNS


PROCERA® ALUMINA/ZIRCONIA, CERCON® ZIRCONIA, LAVA® ZIRCONIA

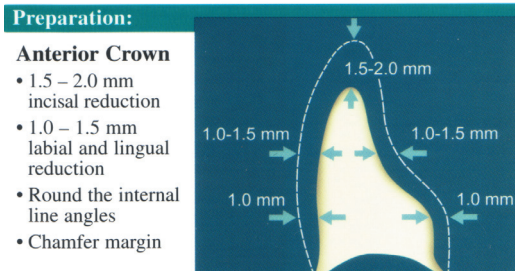

ANTERIOR BRIDGES

PROCERA® ALUMINA/ZIRCONIA, CERCON® ZIRCONIA, LAVA® ZIRCONIA

Note: Bridge connectors must be a minimum of 4.0 mm × 4.0 mm (16-mm sq.)

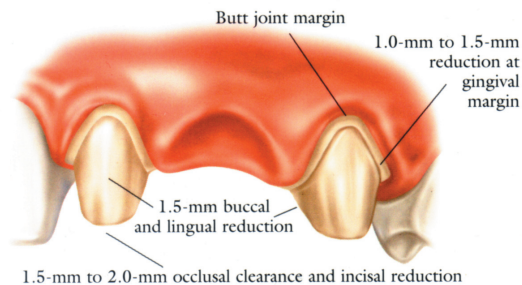

To assure clinical success, the following minimum material thickness is recommended. All prepared surfaces must be rounded on all metal-free restorations.